

Figure 1: Raw count rate curves of SGR 1806-20 recorded by the detector unit no. 0. The vertical dashed line marks the trigger time by Swift/BAT.

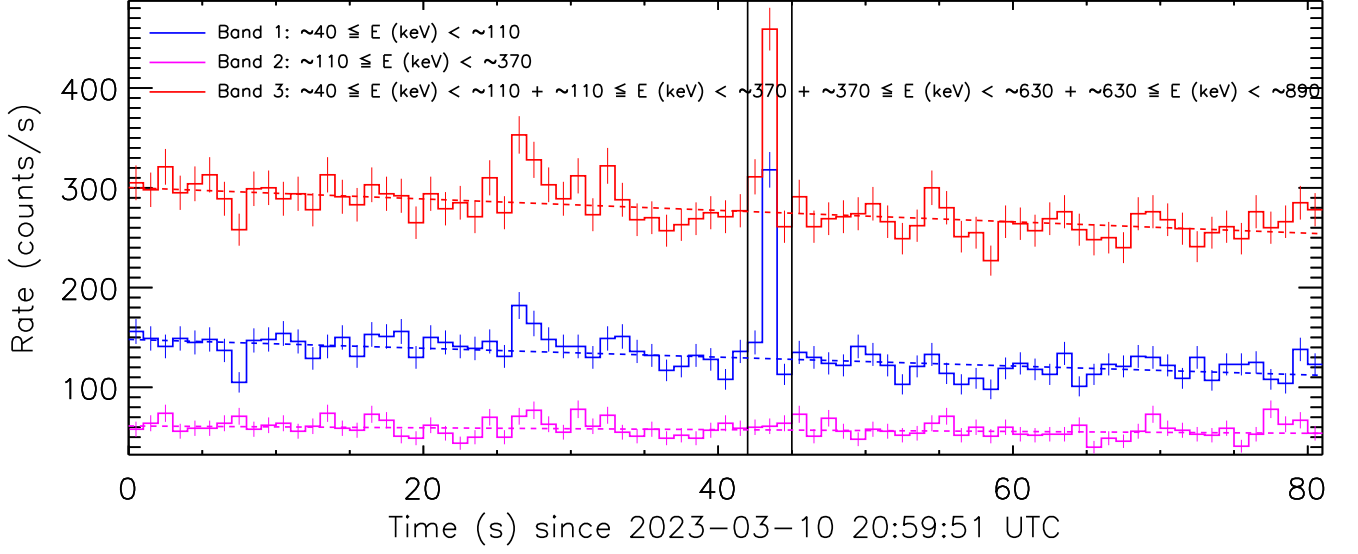


Figure 2: Background fit to the data from the detector unit no. 0 by a linear function. Pre-burst and post-burst intervals which were used for the background fit are delimited by the vertical solid lines.

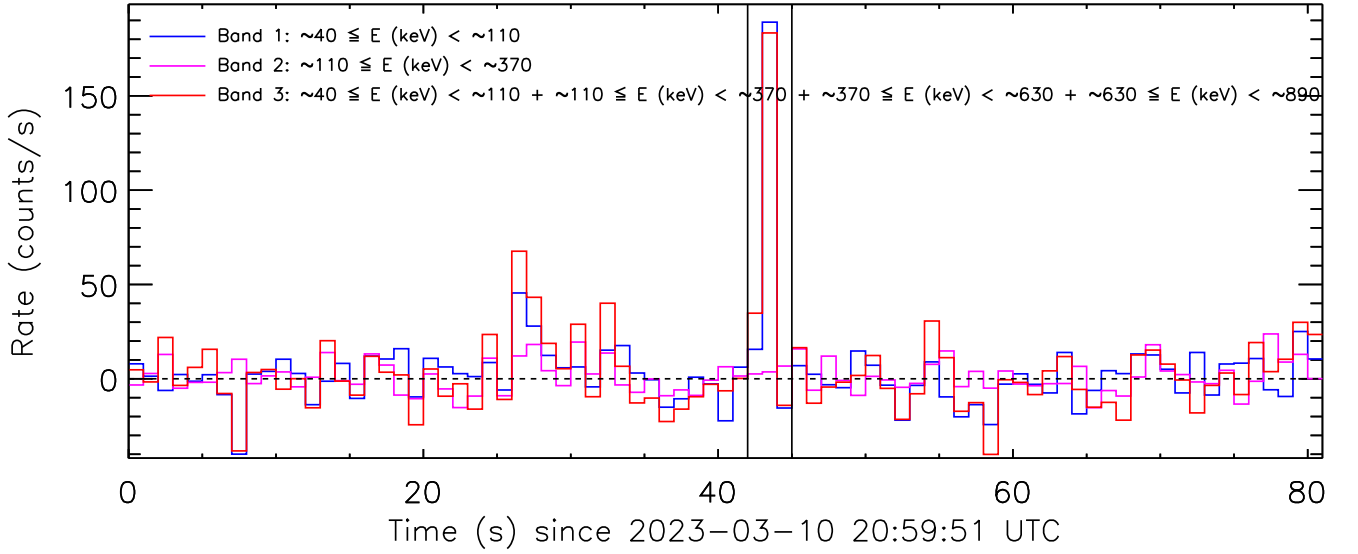


Figure 3: Background-subtracted count rate curves from the detector unit no. 0.

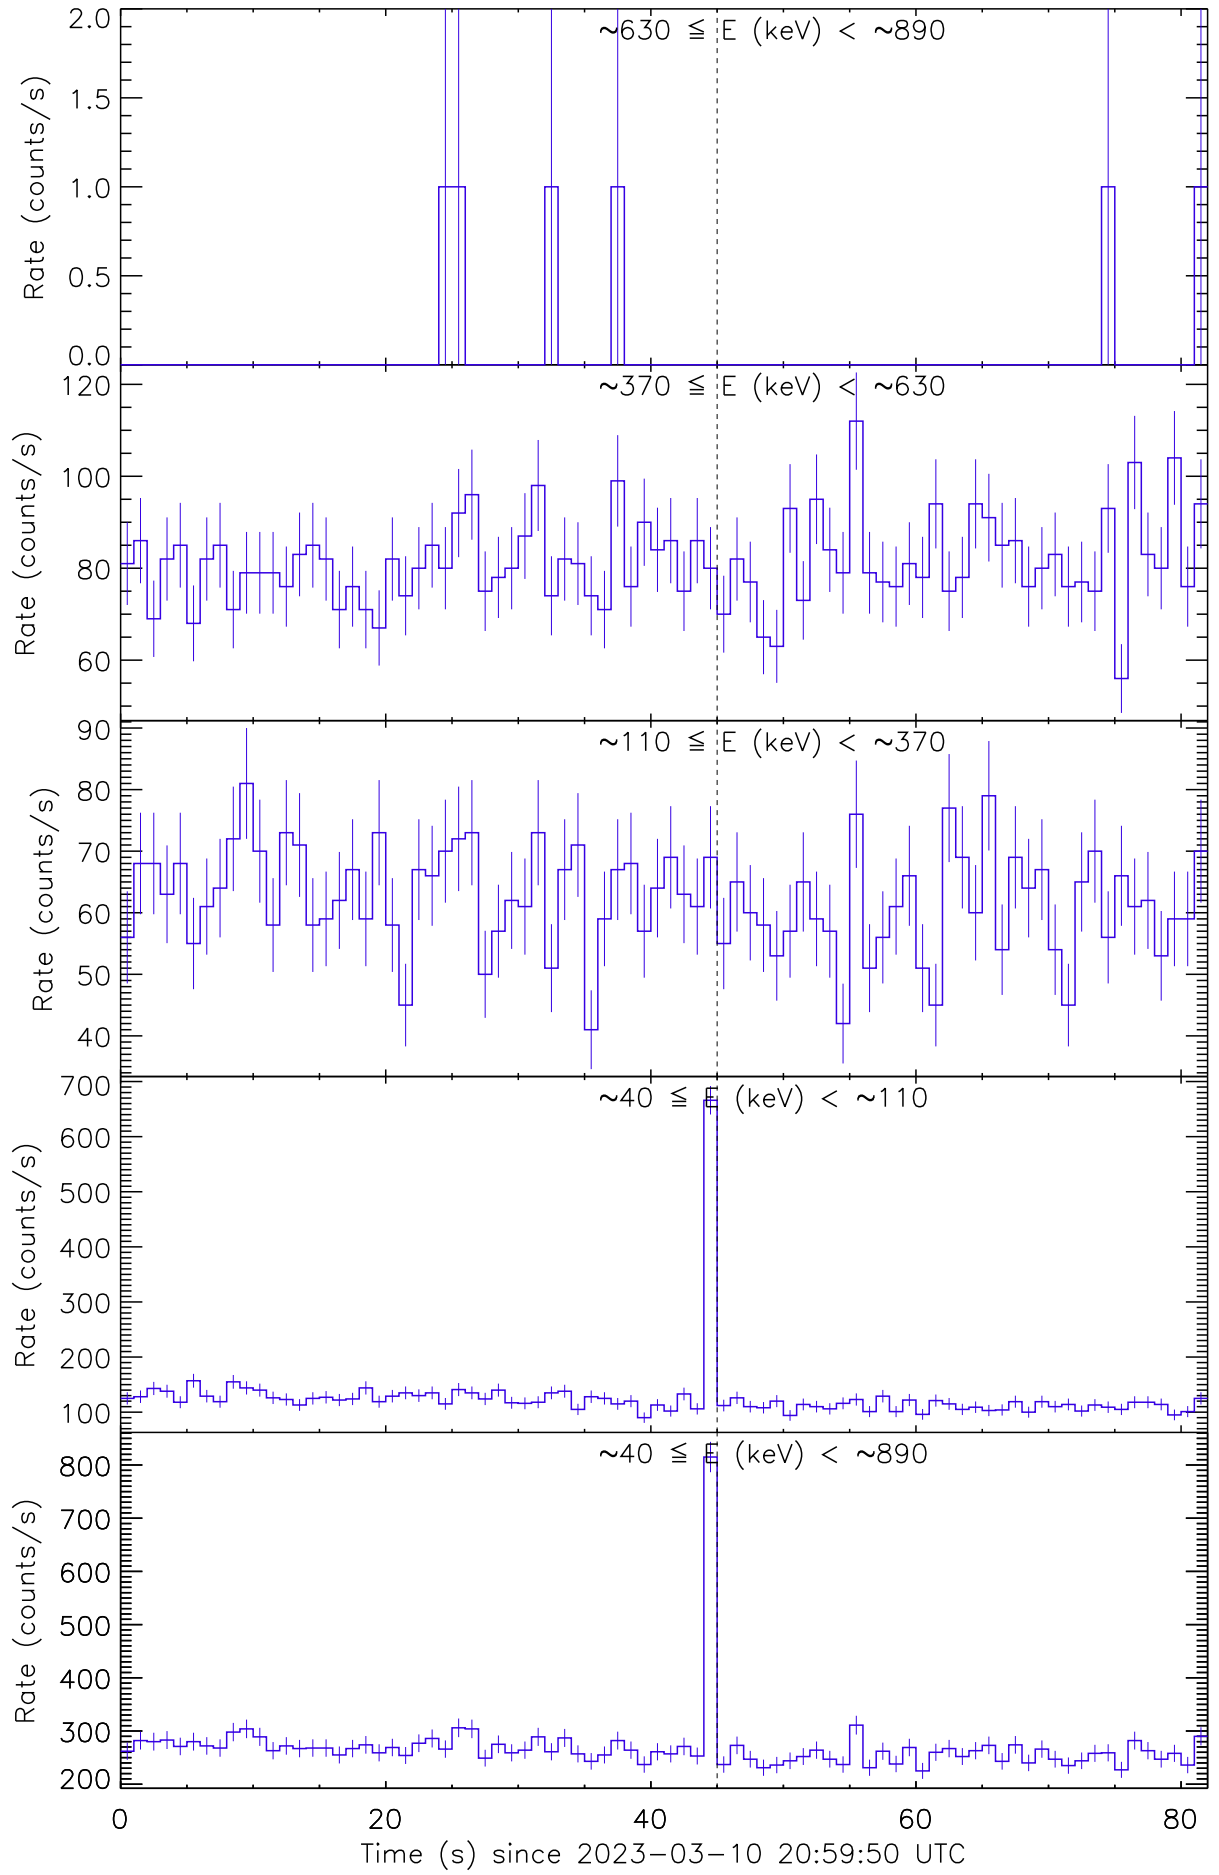


Figure 4: Raw count rate curves of SGR 1806-20 recorded by the detector unit no. 1. The vertical dashed line marks the trigger time by Swift/BAT.

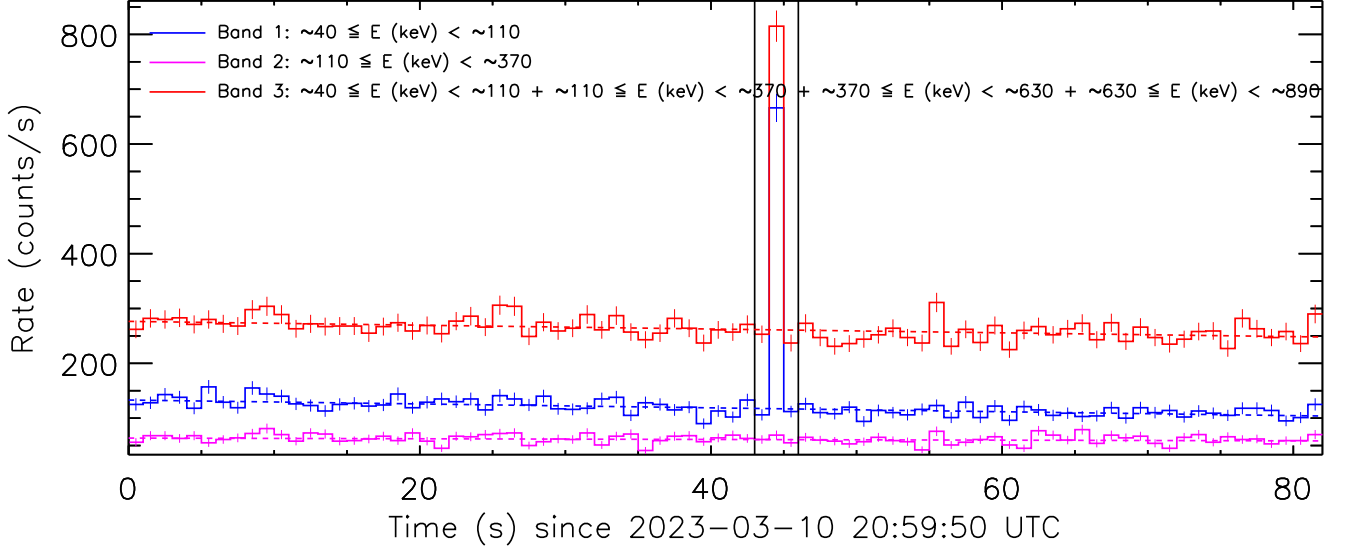


Figure 5: Background fit to the data from the detector unit no.1 by a linear function. The pre-burst and post-burst intervals which were used for the background fit are delimited by the vertical solid lines.

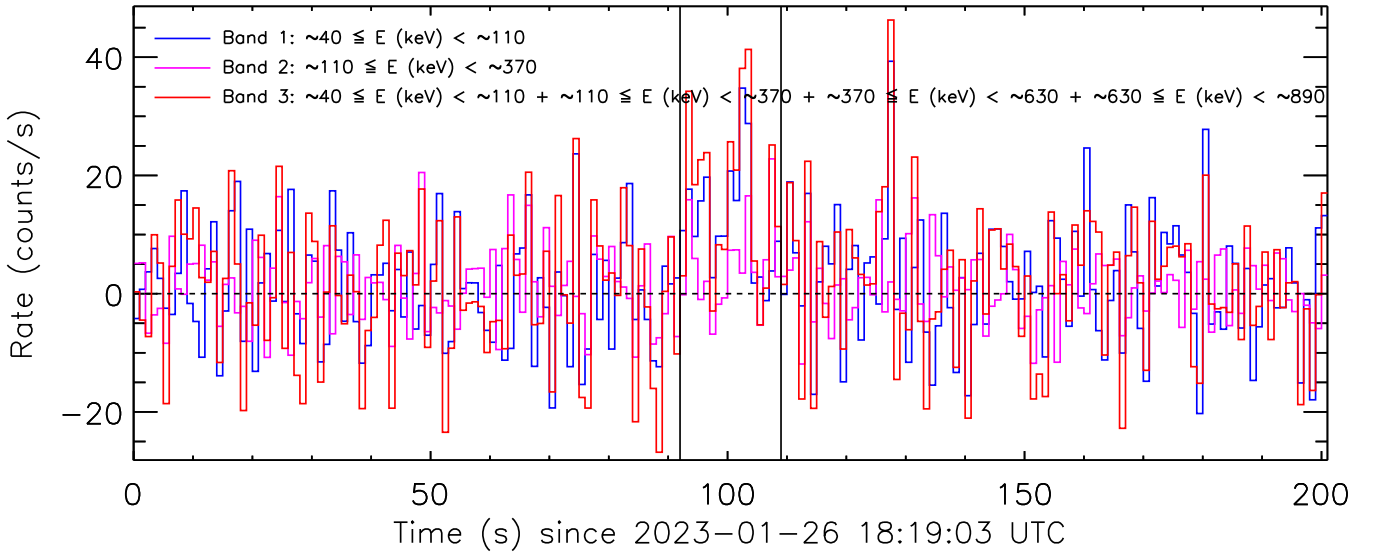


Figure 6: Background-subtracted count rate curves from the detector unit no. 1.